

# NASA TECH BRIEF

## *Lewis Research Center*



NASA Tech Briefs announce new technology derived from the U.S. space program. They are issued to encourage commercial application. Tech Briefs are available on a subscription basis from the National Technical Information Service, Springfield, Virginia 22151. Requests for individual copies or questions relating to the Tech Brief program may be directed to the Technology Utilization Office, NASA, Code KT, Washington, D.C. 20546.

### USE OF SMALL TURBINE-TYPE FLOWMETERS TO MEASURE FLOW IN LARGE PIPES

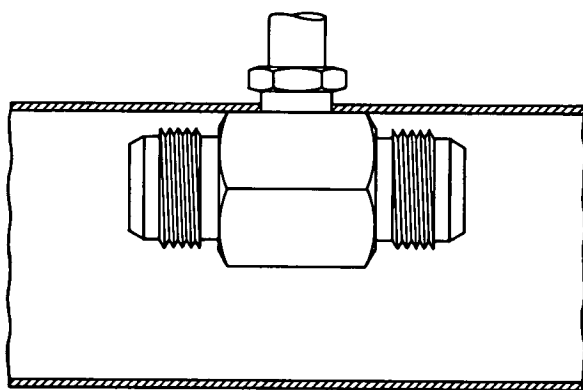


Figure 1. - 2.54-cm Turbine Meter in 7.62-cm Pipe.

Small turbine-type flowmeters have been used in large pipes as velocity detection devices to determine total mass flow in the pipes. The method allows the use of small, inexpensive, and easily calibrated flowmeters to determine mass flow in large pipes in lieu of larger, more expensive flowmeters.

Feasibility experiments were conducted with liquid hydrogen, but the results are applicable to all liquids. A calibrated one-inch diameter turbine-type flowmeter was placed in a three-inch diameter pipe. The flowmeter was placed in the position shown in Figure 1 primarily for convenience. Consideration, however, was given to the velocity profile in the pipe, and the meter was positioned to measure an average velocity. Velocities measured by the flowmeter were consistently slightly higher than the actual average velocities in the pipe, however, as shown in Figure 2. This higher result is attributed to (1) distortion of the velocity profile by the meter, and (2) systematic shift of the average-velocity radius with bulk velocity. The first effect would diminish as pipe size increased. The second effect can be accounted for by assigning a flow coefficient for the installation. A calibration of each installation is therefore necessary.

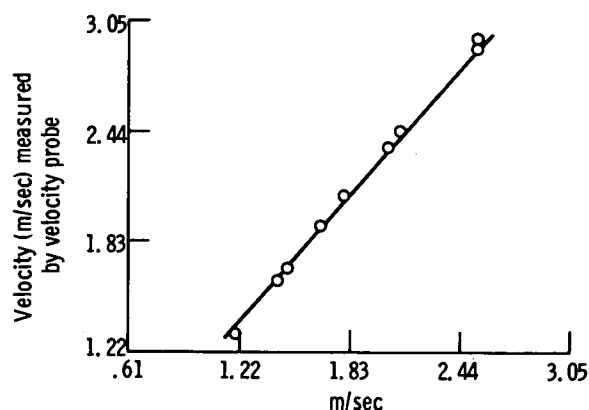


Figure 2. - Velocity (m/sec) measured by calibration facility.

The experiments conducted show the method to be feasible and, with further attention to design detail and the possible use of multiple detectors, the method should be practical and inexpensive for measuring flow rates in large pipes where the size and cost of metering devices becomes prohibitive.

#### NOTE:

No further documentation is available. Specific questions, however, may be directed to:

Technology Utilization Officer  
Lewis Research Center  
21000 Brookpark Road  
Cleveland, Ohio 44135  
Reference: B72-10631

#### PATENT STATUS:

NASA has decided not to apply for a patent.

Source: H.L. Minkin and H.F. Hobart  
Lewis Research Center  
(LEW-11851)

Category 06